



CERTIFICATE OF ACCREDITATION

ANSI National Accreditation Board

11617 Coldwater Road, Fort Wayne, IN 46845 USA

This is to certify that

Aerospace Testing & Pyrometry, Inc.

**4371 Saratoga Drive
Bethlehem, PA 18020
(and satellite site as listed on the scope)**

has been assessed by ANAB and meets the requirements of international standard

ISO/IEC 17025:2017

while demonstrating technical competence in the field of

CALIBRATION

Refer to the accompanying Scope of Accreditation for information regarding the types of activities to which this accreditation applies

L2446

Certificate Number


ANAB Approval

Certificate Valid Through: 03/04/2021
Version No. 004 Issued: 02/12/2019



This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017. This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).



ANSI National Accreditation Board

SCOPE OF ACCREDITATION TO ISO/IEC 17025:2017

Aerospace Testing & Pyrometry, Inc.

4371 Saratoga Drive
Bethlehem, PA 18020
Andrew Bassett 844-828-7225

CALIBRATION

Valid to: March 4, 2021

Certificate Number: L2446

Electrical – DC/Low Frequency

Parameter / Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method and/or Equipment
	(0 to 75) mV	9.3 μ V + 6 μ V/V	Millivolt simulation with Universal Calibrator per AMS-2750E
	(0 to 10) V	6.4 mV + 1 mV/V	Voltage simulation with Universal Calibrator per AMS-2750E
	(0 to 20) mA	9.4 μ A + 2 μ A/A	Milliamp simulation with Universal Calibrator per AMS-2750E
	Pt 100-385 (-320 to 1400) °F	0.71 °F	RTD simulation with Universal Calibrator per AMS-2750E
Calibration of Process instruments ¹	Type B (1 112 to 1 652) °F (1 652 to 2 102) °F (2 102 to 3 000) °F	2.5 °F 1.8 °F 1.5 °F	Thermocouple simulation with Universal Calibrator per AMS-2750E
	Type E (-200 to 1 600) °F	0.69 °F	
	Type J (0 to 932) °F (932 to 1 600) °F	0.68 °F 0.8 °F	
	Type K (-200 to 1 922) °F (1 922 to 2 400) °F	0.8 °F 0.89 °F	
	Type N (0 to 2 012) °F (2 012 to 2 372) °F	0.8 °F 0.89 °F	



ANSI National Accreditation Board

Electrical – DC/Low Frequency

Parameter / Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method and/or Equipment
Calibration of Process instruments ¹	Type R (0 to 482) °F (482 to 1 382) °F (1 382 to 2 192) °F (2 192 to 3 200) °F Type S (0 to 212) °F (212 to 752) °F (752 to 3 092) °F (3 092 to 3 200) °F Type T (-320 to -58) °F (-58 to 32) °F (32 to 750) °F	2.7 °F 1.5 °F 1.3 °F 1.5 °F 2.7 °F 1.9 °F 1.5 °F 1.8 °F 1.3 °F 0.8 °F 0.68 °F	Thermocouple simulation with Universal Calibrator per AMS-2750E

Thermodynamic

Parameter / Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method and/or Equipment
System Accuracy Tests ¹	Type T (-320 to 0) °F (0 to 400) °F Type J (100 to 302) °F (302 to 1 000) °F	2.4 °F 2.1 °F 1.8 °F 1.7 °F	Universal Calibrator/Multipoint Data Logger per AMS-2750E
System Accuracy Tests ¹	Type K (100 to 248) °F (248 to 1 600) °F (1 600 to 2 502) °F Type N (100 to 248) °F (248 to 1 400) °F (1 400 to 2 372) °F	1.8 °F 1.8 °F 2.9 °F 2 °F 2.1 °F 3.2 °F	Universal Calibrator/Multipoint Data Logger per AMS-2750E
Temperature Uniformity Surveys ¹	Type T (-320 to 0) °F (0 to 400) °F Type J (100 to 248) °F (248 to 1 000) °F	2.4 °F 2.1 °F 1.8 °F 1.7 °F	Universal Calibrator/Multipoint Data Logger per AMS-2750E



ANSI National Accreditation Board

Thermodynamic

Parameter / Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method and/or Equipment
Temperature Uniformity Surveys ¹	Type K (100 to 248) °F (248 to 1 600) °F (1 600 to 2 502) °F Type N (100 to 248) °F (248 to 1 400) °F (1 400 to 2 372) °F	1.8 °F 1.8 °F 2.9 °F 2 °F 2.1 °F 3.1 °F	Universal Calibrator/Multipoint Data Logger per AMS-2750E

Work performed at satellite location
Aerospace Testing & Pyrometry, Inc. Calibration Lab
825 Archer Road
Bedford, OH 44146
Dale T. Praznik 844-828-7225

Electrical – DC/Low Frequency


Parameter / Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method and/or Equipment
DC Current – Source ²	(0 to 100) mA	7 µA + 1 µA/A	Calibration by Comparison to Fluke 7526A Calibrator
DC Current – Measure ²	(0 to 100) mA	5.6 µA + 0.5 µA/A	Calibration by Comparison to Keysight 3458A-002
RTD Temperature Meters ²	Pt 385 100Ω - Source (-328 to 1 472) °F PT 385 100 Ω - Measure (-328 to -112) °F (-112 to 212) °F (212 to 752) °F (752 to 1 116) °F (1 116 to 1 472) °F	0.15 °F 0.11 °F 0.09 °F 0.1 °F 0.1 °F 0.11 °F	Calibration by Comparison to Fluke 7526A Calibrator
DC Volts – Source ²	(0 to 100) mV (0 to 1) V (1 to 10) V (10 to 100) V	4 µV + 3 µV/V 38 µV + 10 µV/V 0.38 mV + 100 µV/V 3.8 mV + 1 mV/V	Calibration by Comparison to Fluke 7526A Calibrator



ANSI National Accreditation Board

Electrical – DC/Low Frequency

Parameter / Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method and/or Equipment
DC Volts – Measure ²	(0 to 100) mV (0 to 1) V (1 to 10) V (10 to 100) V	1.5 μ V + 0.3 μ V/V 6.6 μ V + 0.3 μ V/V 88 μ V + 0.5 μ V/V 0.8 mV + 30 μ V/V	Calibration by Comparison to Keysight 3458A-002

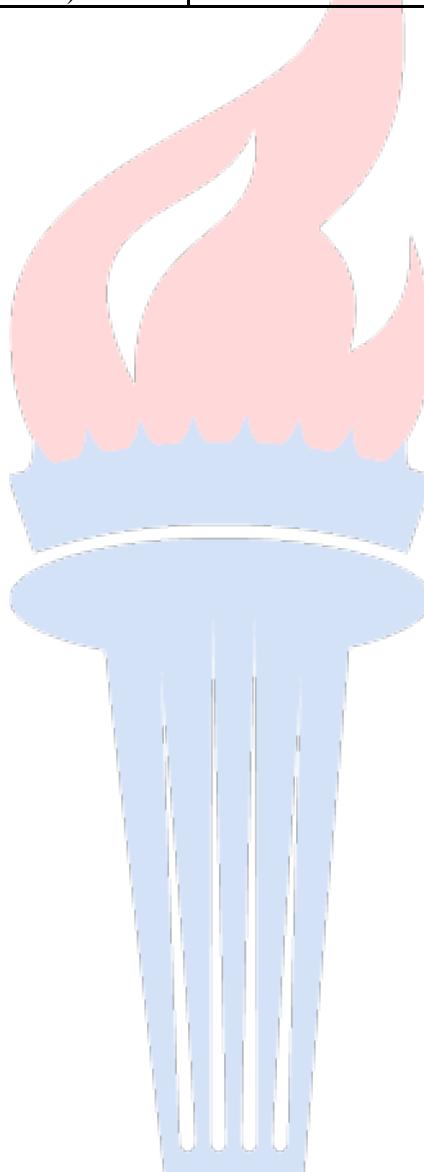



ANSI National Accreditation Board

Thermocouple Indicators - Source ²	Type B (392 to 572) °F (572 to 1 112) °F (1 112 to 1 472) °F (1 472 to 2 822) °F (2 822 to 3 308) °F	0.62 °F 0.52 °F 0.76 °F 0.61 °F 0.5 °F	Calibration by Comparison to Fluke 7526A Calibrator
	Type C (32 to 1 832) °F (1 832 to 3 272) °F (3 272 to 3 632) °F (3 632 to 4 201) °F	0.38 °F 0.52 °F 0.58 °F 0.76 °F	
	Type E (-418 to -328) °F (-328 to -148) °F (-148 to 32) °F (32 to 1 112) °F (1 112 to 1 832) °F	0.55 °F 0.3 °F 0.24 °F 0.23 °F 0.27 °F	
	Type J (-346 to -148) °F (-148 to 1 472) °F (1 472 to 2 192) °F	0.34 °F 0.24 °F 0.27 °F	
	Type K (-418 to -328) °F (-328 to -148) °F (-148 to 932) °F (932 to 1 472) °F (1 472 to 2 502)	0.98 °F 0.37 °F 0.27 °F 0.26 °F 0.32 °F	
	Type N (-418 to -328) °F (-328 to -148) °F (-148 to 32) °F (32 to 932) °F (932 to 1 472) °F (1 472 to 2 372) °F	1.6 °F 0.51 °F 0.3 °F 0.29 °F 0.28 °F 0.31 °F	
	Type R (-58 to -13) °F (-13 to 32) °F (32 to 212) °F (212 to 752) °F (752 to 1 112) °F (1 112 to 1 832) °F (1 832 to 2 912) °F (2 912 to 3 213) °F	1.2 °F 0.96 °F 0.83 °F 0.61 °F 0.5 °F 0.48 °F 0.44 °F 0.51 °F	
	Type S (-58 to -13) °F (-13 to 32) °F	1.1 °F 0.91 °F	
Thermocouple Indicators - Source ²			Calibration by Comparison to Fluke 7526A Calibrator



ANSI National Accreditation Board

Electrical – DC/Low Frequency

Parameter / Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method and/or Equipment
	(32 to 212) °F (212 to 752) °F (752 to 1 112) °F (1 112 to 1 832) °F (1 832 to 2 912) °F (2 912 to 3 213) °F	0.81 °F 0.63 °F 0.51 °F 0.5 °F 0.5 °F 0.58 °F	
	Type T (-418 to -326) °F (-326 to -148) °F (-148 to 32) °F (32 to 392) °F (392 to 752) °F	0.75 °F 0.37 °F 0.28 °F 0.25 °F 0.24 °F	
	Type B (392 to 572) °F (572 to 1 112) °F (1 112 to 1 472) °F (1 472 to 2 822) °F (2 822 to 3 308) °F	0.79 °F 0.72 °F 0.77 °F 0.64 °F 0.53 °F	
	Type C (32 to 1 832) °F (1 832 to 3 272) °F (3 272 to 3 632) °F (3 632 to 4 201) °F	0.39 °F 0.58 °F 0.63 °F 0.8 °F	
Thermocouple Calibrators - Measure ²	Type E (-418 to -328) °F (-328 to -148) °F (-148 to 32) °F (32 to 1 112) °F (1 112 to 1 832) °F	0.54 °F 0.28 °F 0.22 °F 0.2 °F 0.26 °F	Calibration by Comparison to Fluke 7526A Calibrator
	Type J (-346 to -148) °F (-148 to 1 472) °F (1 472 to 2 192) °F	0.32 °F 0.22 °F 0.25 °F	
	Type K (-418 to -328) °F (-328 to -148) °F (-148 to 932) °F (932 to 1 472) °F (1 472 to 2 502)	0.97 °F 0.36 °F 0.25 °F 0.25 °F 0.31 °F	



ANSI National Accreditation Board

ANAB

Electrical – DC/Low Frequency

Parameter / Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method and/or Equipment
Thermocouple Calibrators – Measure ²	Type N (-418 to -328) °F (-328 to -148) °F (-148 to 32) °F (32 to 932) °F (932 to 1 472) °F (1 472 to 2 372) °F Type R (-58 to -13) °F (-13 to 32) °F (32 to 212) °F (212 to 752) °F (752 to 1 112) °F (1 112 to 1 832) °F (1 832 to 2 912) °F (2 912 to 3 213) °F Type S (-58 to -13) °F (-13 to 32) °F (32 to 212) °F (212 to 752) °F (752 to 1 112) °F (1 112 to 1 832) °F (1 832 to 2 912) °F (2 912 to 3 213) °F Type T (-418 to -326) °F (-326 to -148) °F (-148 to 32) °F (32 to 392) °F (392 to 752) °F	1.6 °F 0.5 °F 0.29 °F 0.28 °F 0.27 °F 0.3 °F 1.2 °F 0.97 °F 0.84 °F 0.62 °F 0.51 °F 0.49 °F 0.45 °F 0.53 °F 1.1 °F 0.91 °F 0.82 °F 0.64 °F 0.51 °F 0.52 °F 0.52 °F 0.59 °F 0.74 °F 0.36 °F 0.26 °F 0.21 °F 0.22 °F	Calibration by Comparison to Fluke 7526A Calibrator

Calibration and Measurement Capability (CMC) is expressed in terms of the measurement parameter, measurement range, expanded uncertainty of measurement and reference standard, method, and/or equipment. The expanded uncertainty of measurement is expressed as the standard uncertainty of the measurement multiplied by a coverage factor of 2 ($k=2$), corresponding to a confidence level of approximately 95%.



ANSI National Accreditation Board

Notes:

1. On-site calibration service is available for this parameter, since on-site conditions are typically more variable than those in the laboratory, larger measurement uncertainties are expected on-site than what is reported on the accredited scope.
2. Laboratory offers calibration services for Secondary Standard and Field Test Instruments at the laboratory's own facilities per the requirements of AMS 2750 E
3. This scope is formatted as part of a single document including Certificate of Accreditation No. L2466.



Vice President

